

VistaScan View


Kurzanleitung

Die folgenden Informationen sind eine Ergänzung zur Montage- und Gebrauchsanweisung des Gerätes.


Grundsätzlich ist zusätzlich die Montage- und Gebrauchsanweisung des Gerätes zu beachten, in der wichtige Informationen wie z. B. Sicherheitshinweise, Aufstellung, elektrischer Anschluss, Desinfektion, Reinigung, etc. beschrieben sind.

1 Bilddaten auslesen über Computer - intraoral


1.

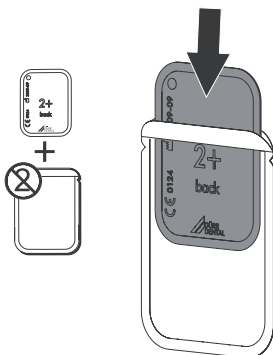


2.

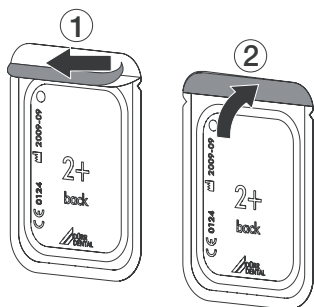


3.

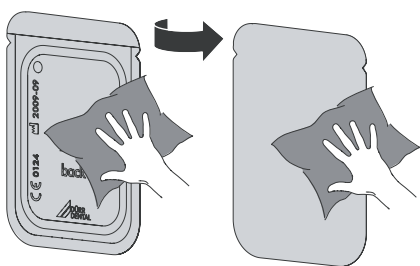


4.

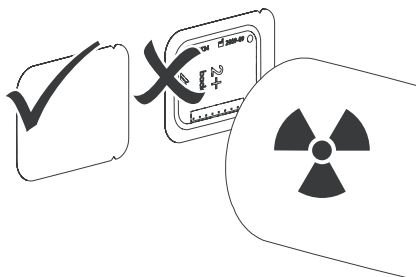


5.

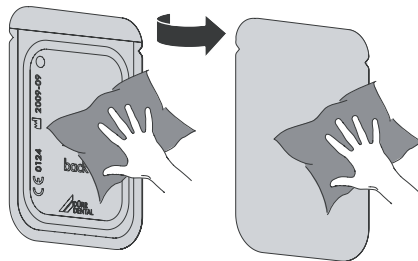


6.

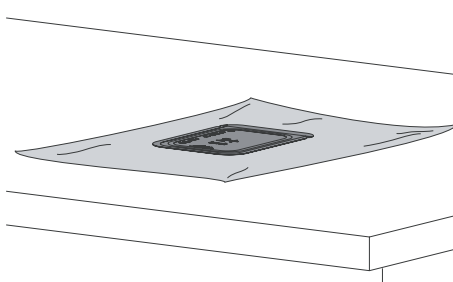


7.



8.




9.

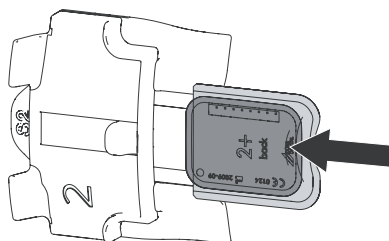


10.




11.

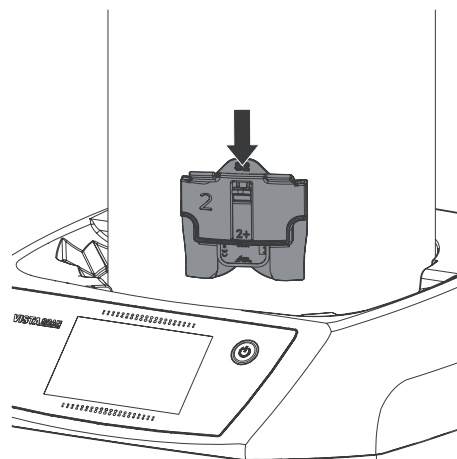

12.

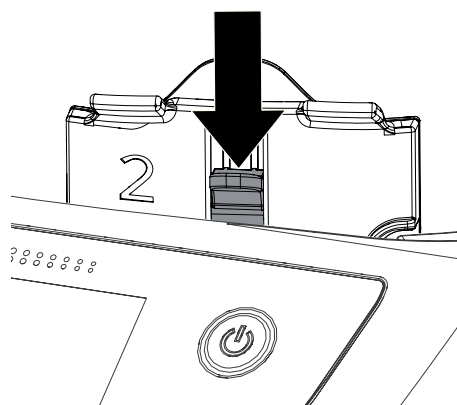

13.

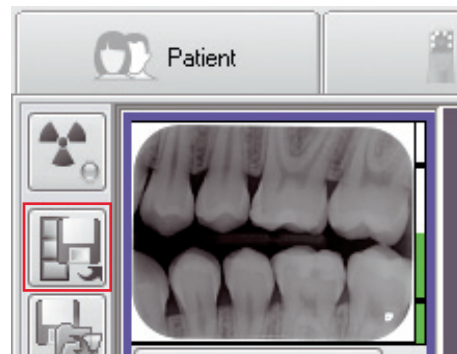

VistaScan View


Kurzanleitung

Die folgenden Informationen sind eine Ergänzung zur Montage- und Gebrauchsanweisung des Gerätes.


Grundsätzlich ist zusätzlich die Montage- und Gebrauchsanweisung des Gerätes zu beachten, in der wichtige Informationen wie z. B. Sicherheitshinweise, Aufstellung, elektrischer Anschluss, Desinfektion, Reinigung, etc. beschrieben sind.

2 Bilddaten auslesen über Touchscreen am Gerät - intraoral


1.

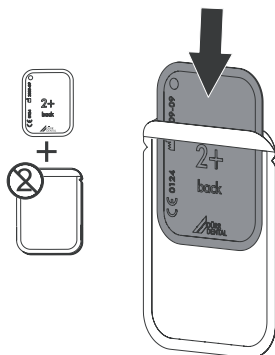


2.

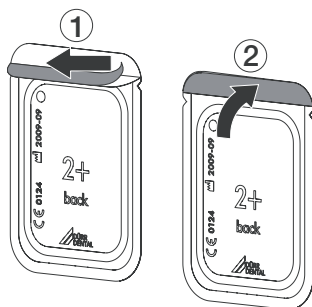


3.

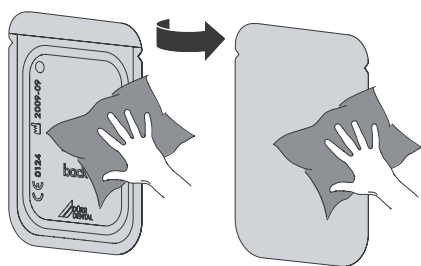


4.

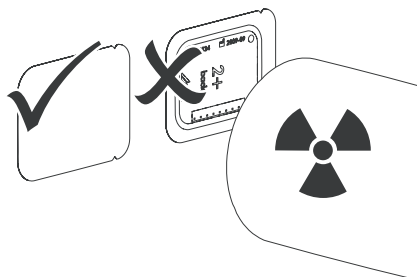


5.

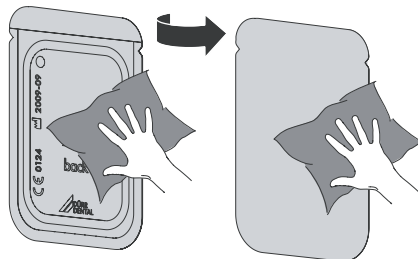


6.

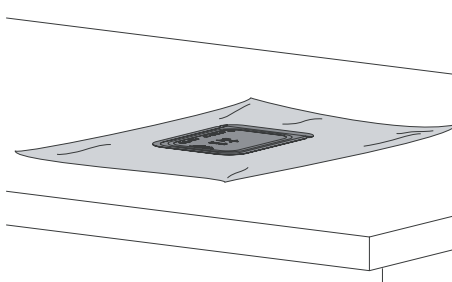


7.



8.




9.

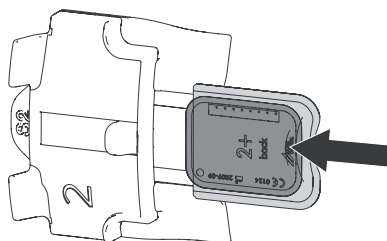


10.



11.

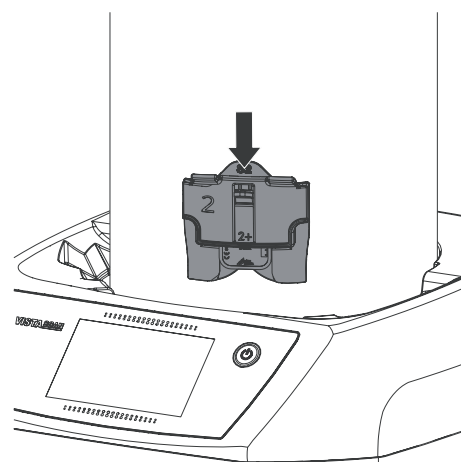

12.

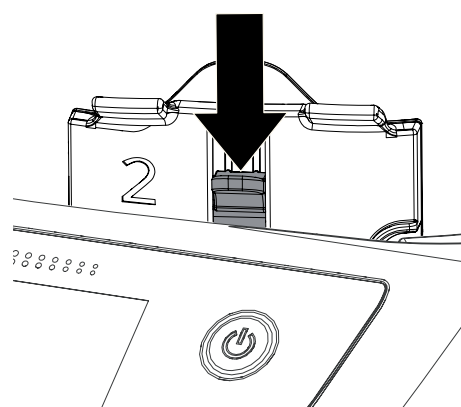

13.



DÜRR DENTAL AG

Höpfigheimer Strasse 17
74321 Bietigheim-Bissingen, Germany

9000-618-209/01




1303V001


DÜRR
DENTAL

3 Bilddaten auslesen über Computer - extraoral


1.

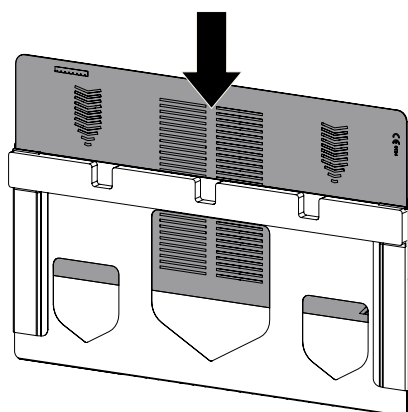

2.

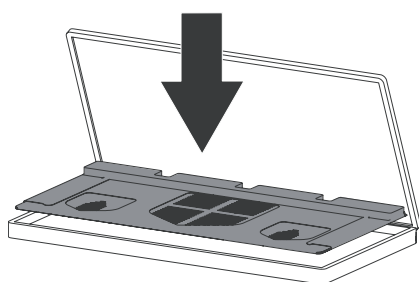


3.

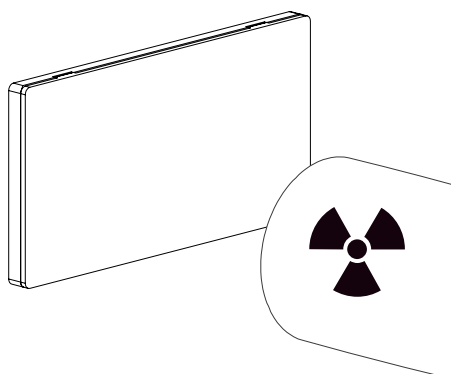


4.




5.

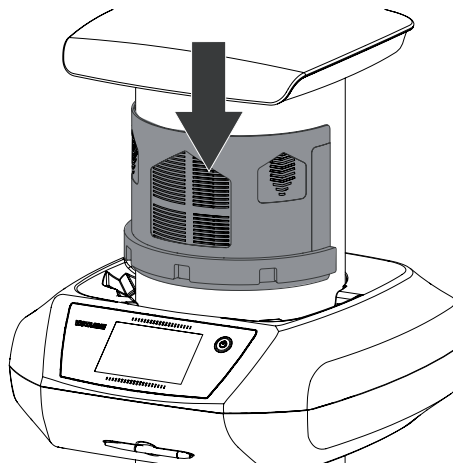

6.

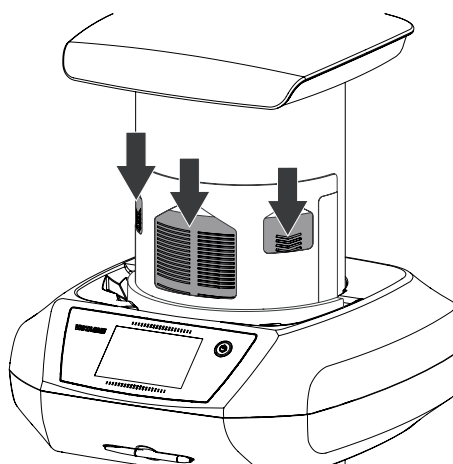


7.

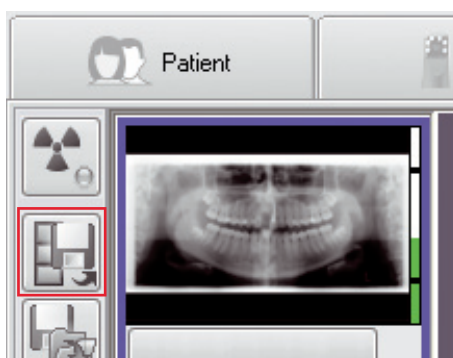


4 Bilddaten auslesen über Touchscreen am Gerät - extraoral


1.

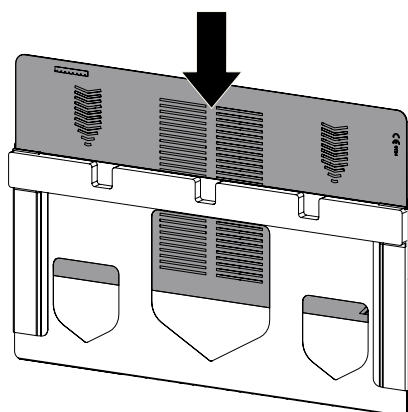

2.

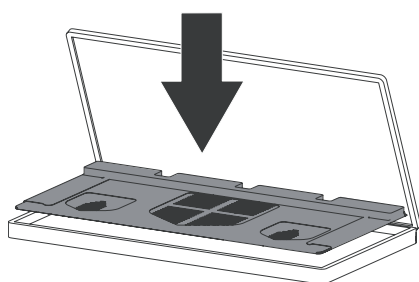


3.

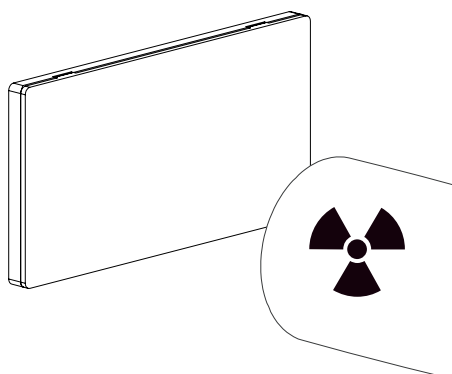


4.




5.

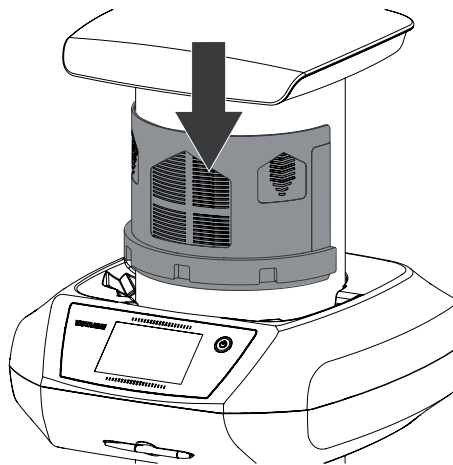

6.

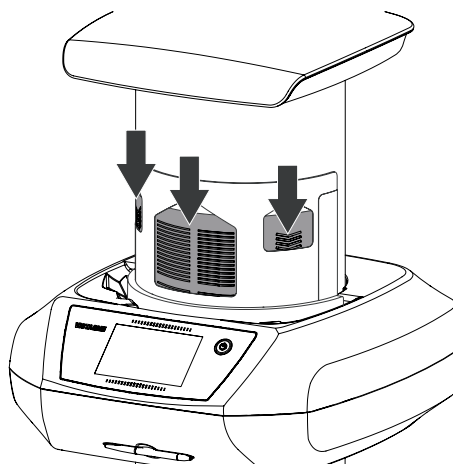

7.

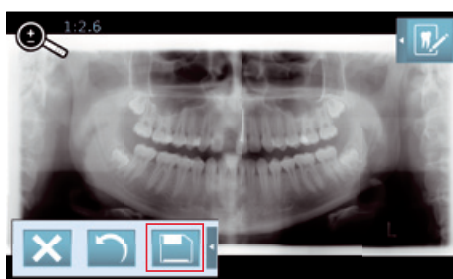

VistaScan View


Short introduction

The following information is supplementary to the appliance Installation and Operating Instructions.


Always refer to the Installation and Operating Instructions of the appropriate appliance in which important information is detailed, e. g. Safety Instructions, Set-up, Electrical Connections, Disinfection, Cleaning, etc.

1 Reading the image data using the computer - intraoral


1.

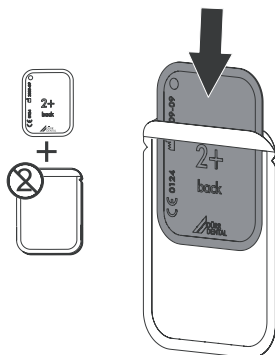


2.

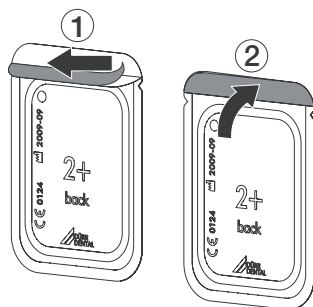


3.

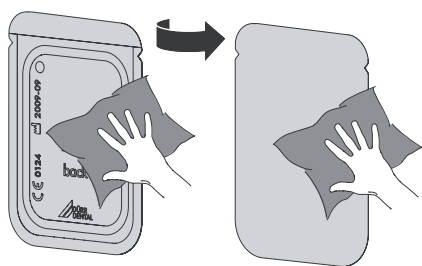


4.

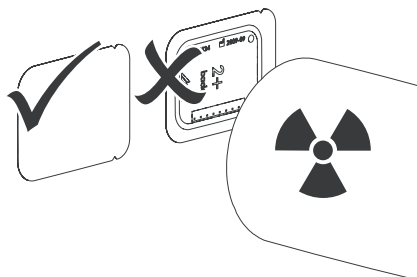


5.

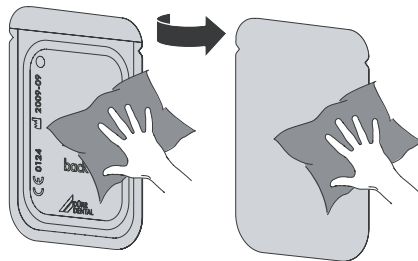


6.

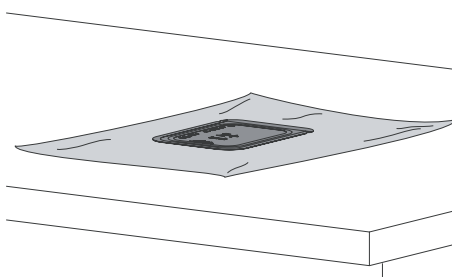


7.



8.




9.

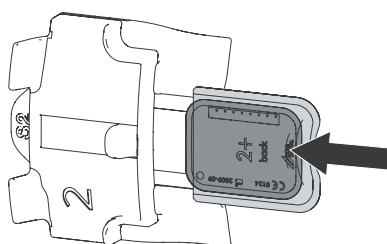


10.




11.

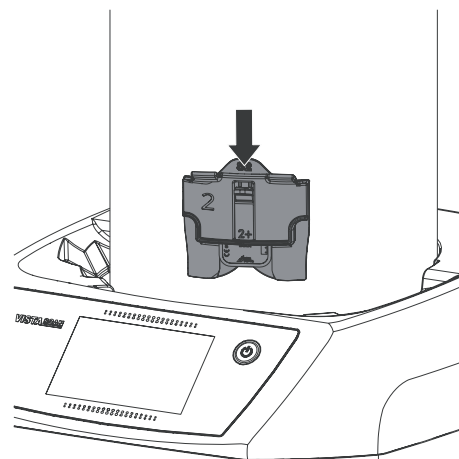

12.

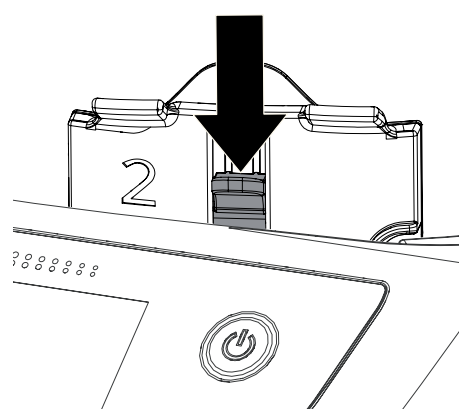

13.

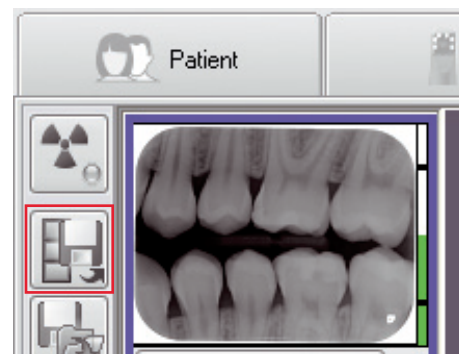

VistaScan View


Short introduction

The following information is supplementary to the appliance Installation and Operating Instructions.


Always refer to the Installation and Operating Instructions of the appropriate appliance in which important information is detailed, e. g. Safety Instructions, Set-up, Electrical Connections, Disinfection, Cleaning, etc.

2 Scanning image data using the unit touch screen - intraoral


1.

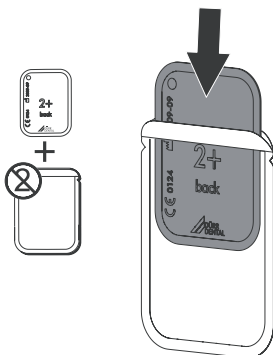


2.

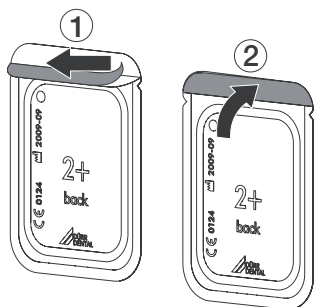


3.

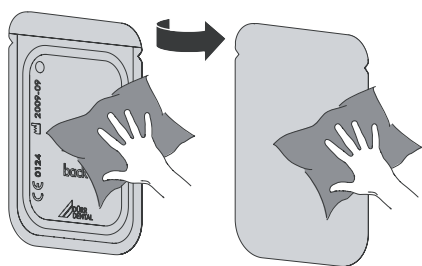


4.

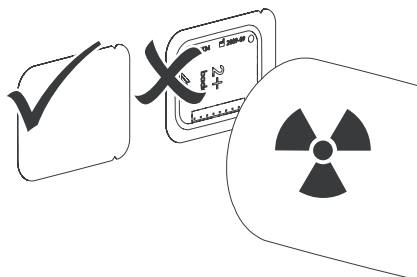


5.

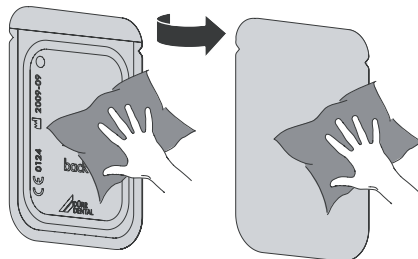


6.

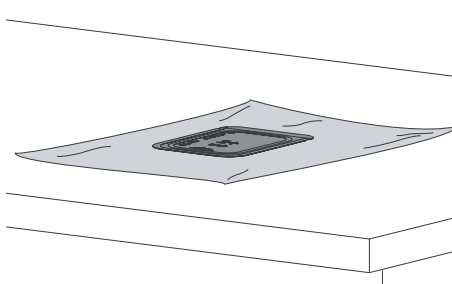


7.



8.




9.

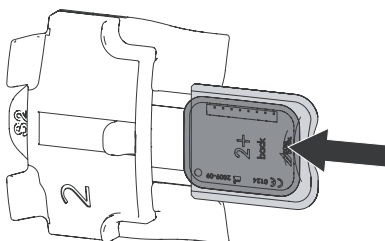


10.



11.

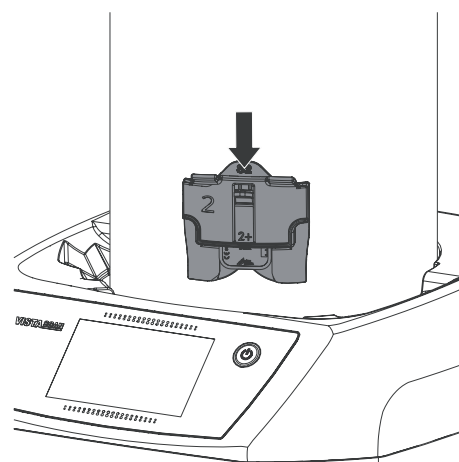

12.

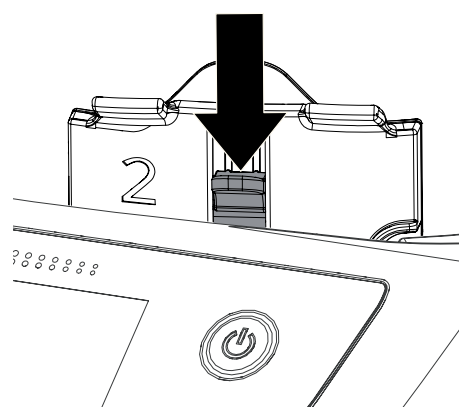

13.



DÜRR DENTAL AG

Höpfheimer Strasse 17
74321 Bietigheim-Bissingen, Germany

9000-618-209/01




1303V001


DÜRR
DENTAL

3 Reading the image data using the computer - extraoral


1.

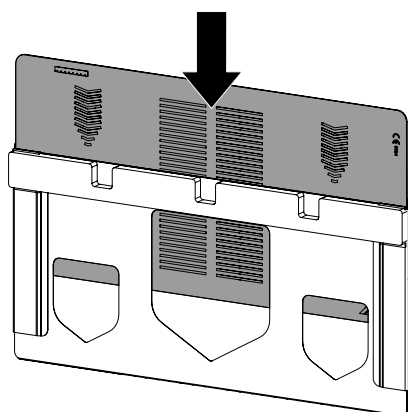

2.

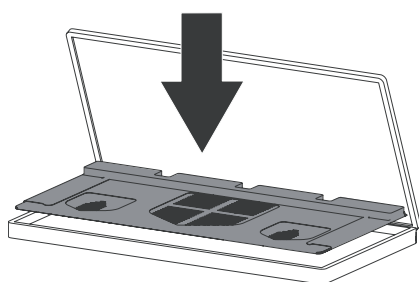


3.

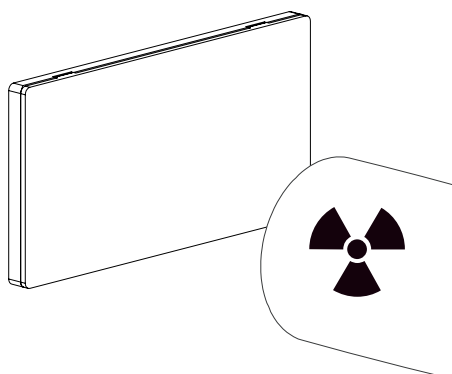


4.




5.

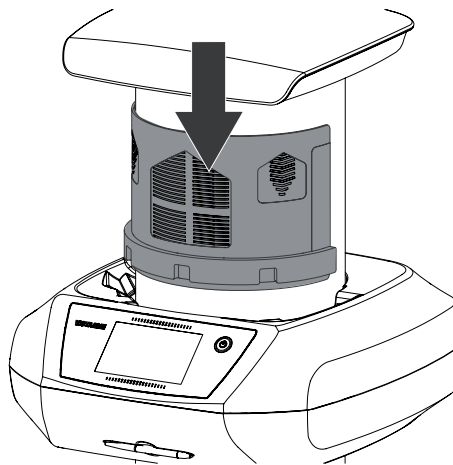

6.

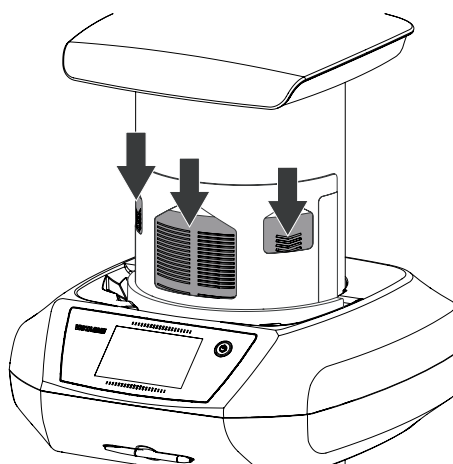


7.

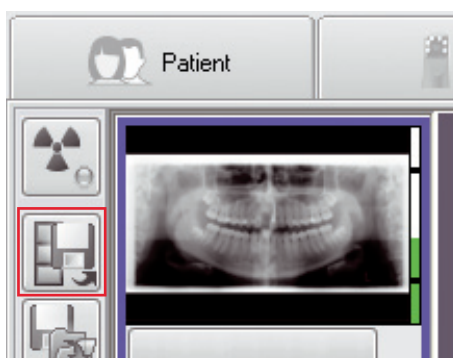


4 Scanning image data using the unit touch screen - extraoral


1.

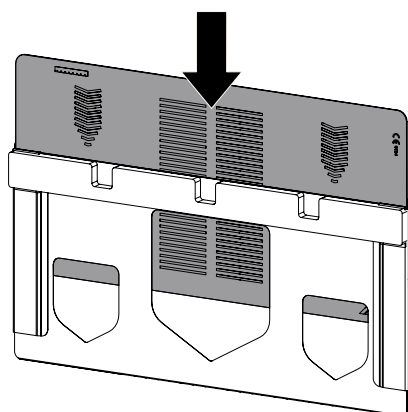

2.

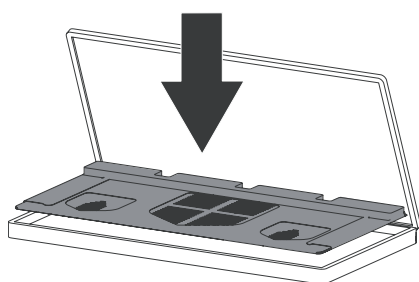


3.

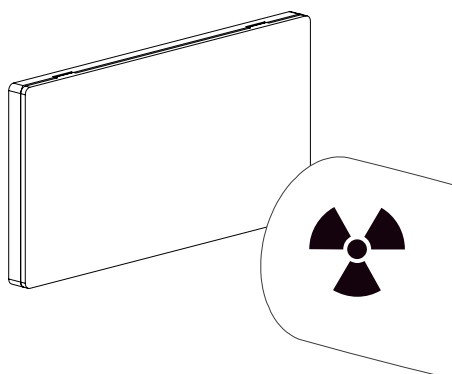


4.



5.

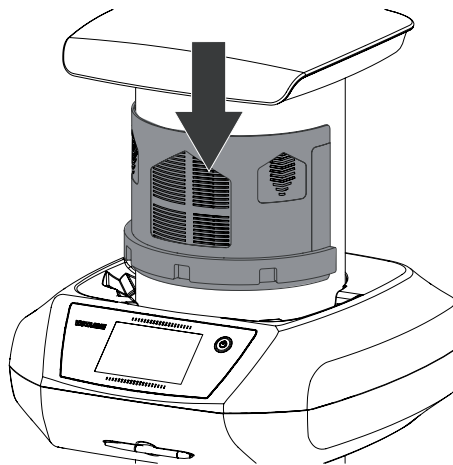

6.

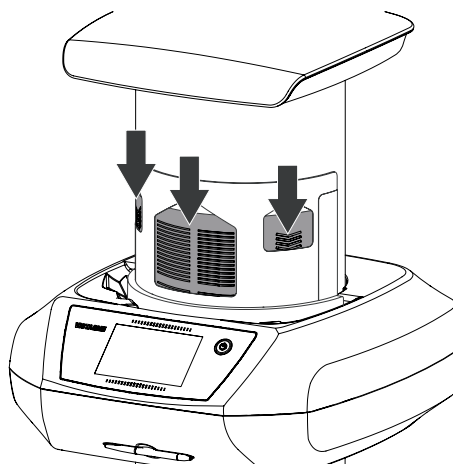

7.

